

ZATA Standard

Name:

DoB:

Date:

Right Rx:.....

Pupil Diameter:OD 3 OS 3

Record number

Age:

Time: 10:23:14 AM

Left Rx:.....

VA: OD OS

Threshold

30/24-2

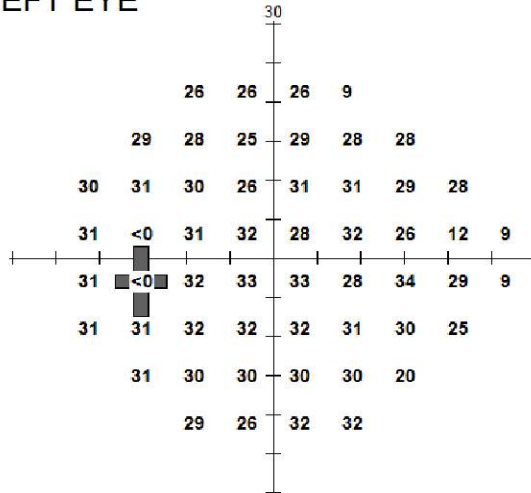
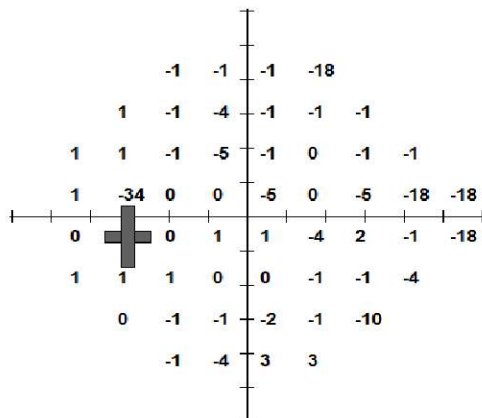
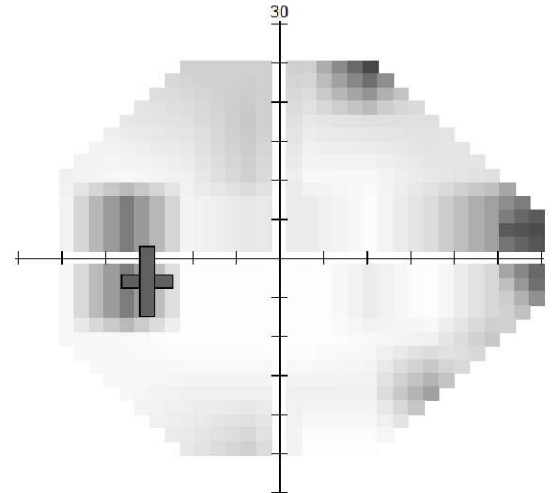
Goldmann III white stimulus

Background 10 cd/m²

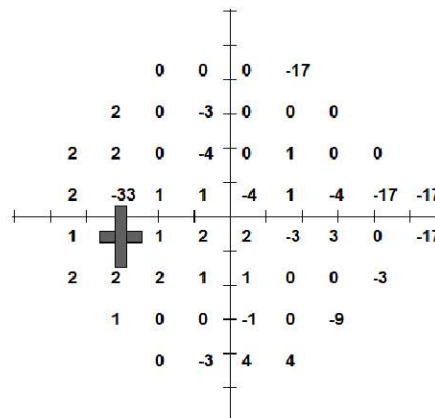
Blindspot Fixation Monitor

Central Fixation

LEFT EYE


Threshold dB (0=3183cd/m²)


Total Defect dB



Pattern Defect dB

Presentations 54
Fovea Off

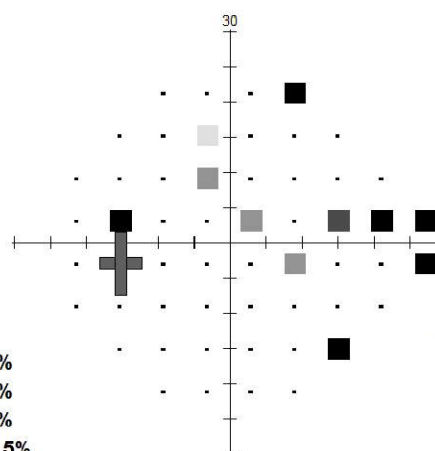
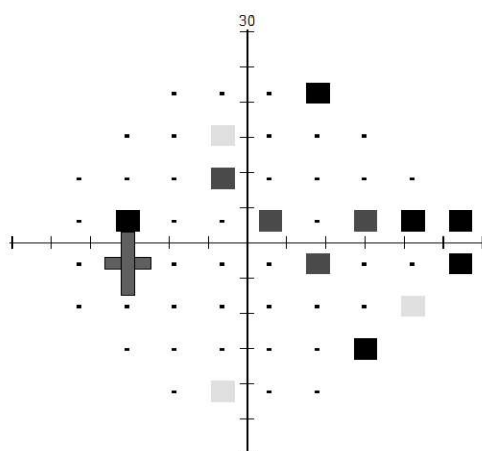
Fixation Losses 0/12

False Positives 0/11

False Negatives 2/9

Mean Defect -1.64 dB
Within normal limits

Std Dev Defect 4.35 dB
p<0.5%

Hemifield Test
Outside normal limits p<0.5%

<5%
<2%
<1%
<0.5%

Henson 9000

Normative database Version 2.0

Software Version 4.0.114